



NOTES:



- LEAD PANELS SHALL BE CONSTRUCTED FROM SINGLE UNPIERCED SHEET, FREE OF OXIDE INCLUSIONS, FISSURES, VOIDS AND ALL OTHER DETRIMENTAL DEFECTS. MATERIAL SHALL BE LEAD GRADE "C" TO COMPLY WITH FEDERAL SPECIFICATION-QQ-L201. CABINET SHALL MEET ALL APPLICABLE FEDERAL, STATE AND LOCAL RADIATION GUIDE LINES: NBS HANDBOOK 111 AND 114, ANS N43.2 AND DOE ORDER 5480.11.
- FINISH - PAINT EXTERIOR SURFACES, EXCEPT AS NOTED, WITH PRATT & LAMBERT #2127 (SNO-FLAKE WHITE, SEMI-GLOSS, EPOXY BASE) OR EQUIVALENT. SURFACE PREPARATION PER A.N.L. SPECIFICATION #4105-000 24.
- DIMENSIONS IN BRACKETS [] ARE MILLIMETERS AND ARE FOR REFERENCE ONLY.
- SOME HIDDEN LINES MAY BE OMITTED FOR CLARITY.

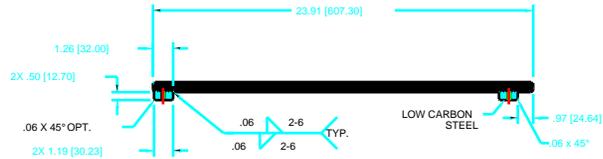

SECTION A-A

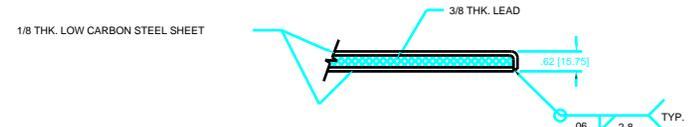


SECTION AROUND PERIMETER

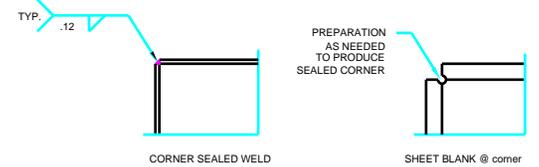

SIDING PREPARATION TYPICAL DETAIL

SCALE= 1:2

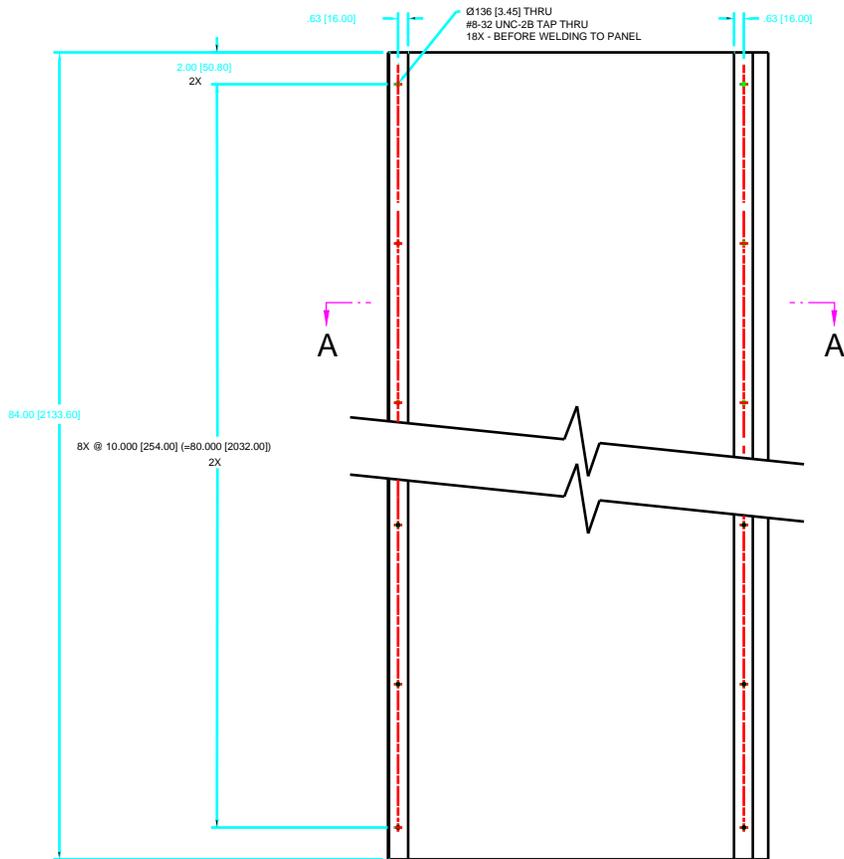

ITEM	QUANTITY	UNIT	DESCRIPTION	MATERIAL / SPEC	REV
PARTS LIST					
<p> ARGONNE NATIONAL LABORATORY HAS BELONGS TO THE PROPERTY OF ADVANCED PHOTON SOURCE U6 ID SHIELDED CABINET SLITS L2 DOOR PANEL </p>					
PART NO: A2244800		DATE: 4/7/95		DRAWN BY: M. KOHUT	
CHECKED BY: SANCHEZ/PATA		DATE: 4/7/95		PROJECT NO:	
SEE NOTES					
SCALE: 1:4				SHEET: D	
P4105090606-200015-00					