
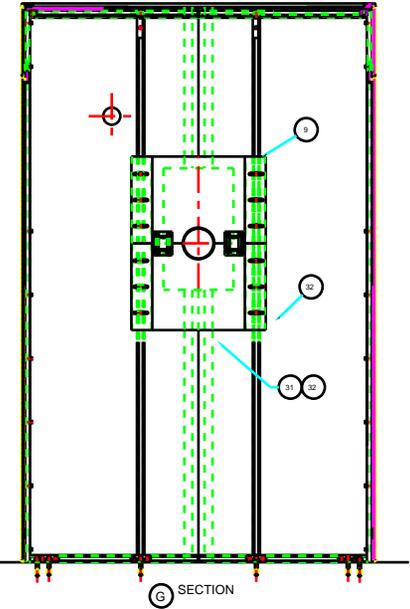
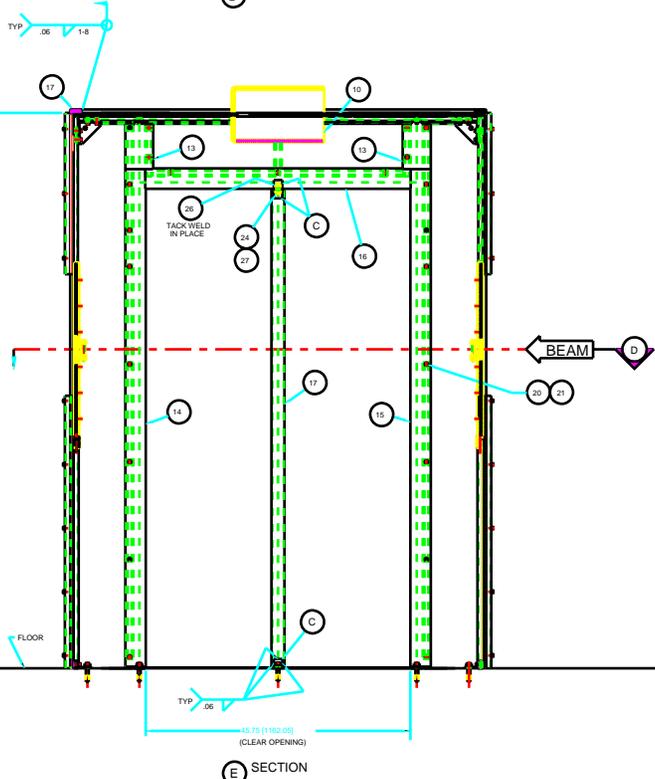
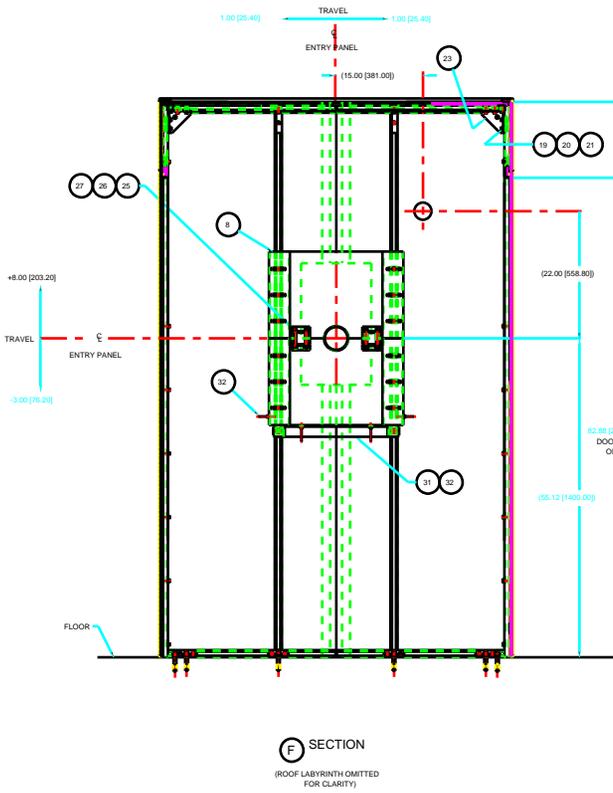
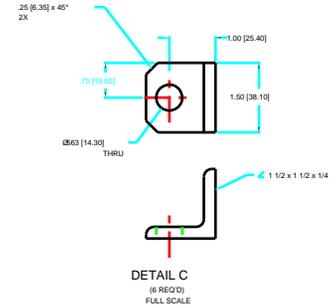
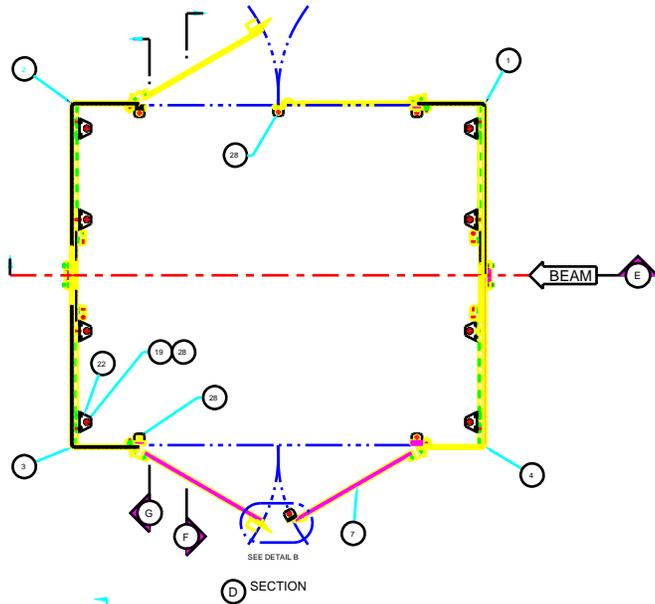


- NOTES:
1. LEAD PANELS SHALL BE CONSTRUCTED FROM SINGLE UNPIERCED SHEET, FREE OF OXIDE INCLUSIONS, FISSURES, VOIDS AND ALL OTHER DETRIMENTAL DEFECTS. MATERIAL SHALL BE LEAD GRADE "C" TO COMPLY WITH FEDERAL SPECIFICATION-00L201. CABINET SHALL MEET ALL APPLICABLE FEDERAL, STATE AND LOCAL RADIATION GUIDE LINES: NBS HANDBOOK 111 AND 114, ANS N43.2 AND DOE ORDER 5480.11.
 2. PAINT EXPOSED LEAD SURFACES PER SPEC. (EXCEPT AS NOTED)
 3. DIMENSIONS IN BRACKETS () ARE MILLIMETERS AND ARE FOR REFERENCE ONLY.
 4. SOME HIDDEN LINES MAY BE OMITTED FOR CLARITY.

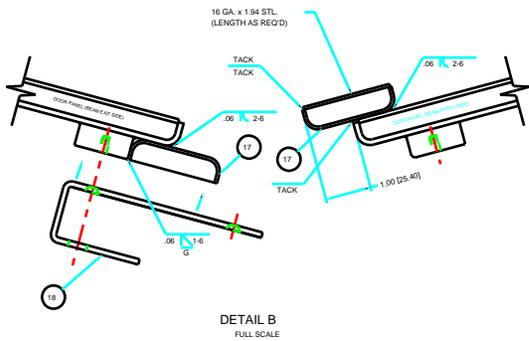

A2289700		ARGONNE NATIONAL LABORATORY	
J.S. PALANCHAR 01/2018	DESIGNED BY	ADVANCED PHOTON SOURCE	
SANCHEZ/PALANCHAR	DESIGNED BY	U6 I6 SHIELDED CABINET L2 & P8 SHUTTER & SLITS ASSEMBLY	
SECTIONS		1/8"=1	P4105090606-600000-00